



Normalize HTRF cytokine assays to cell viability

Measure cytokines using HTRF assays and determine cell viability on a well-by-well or cell-by-cell basis with the EarlyTox™ Cell Integrity Kit on the SpectraMax i3x® Multi-Mode Microplate Reader and the SpectraMax® Minimax™ 300 Imaging Cytometer.


1 PBMC seeding

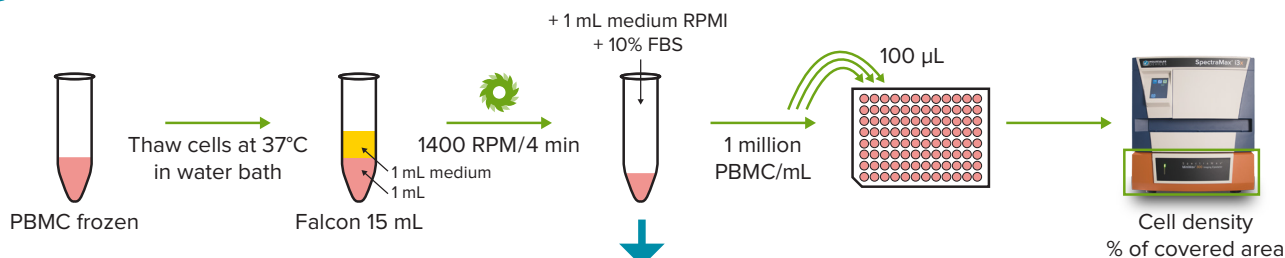


2 PBMC treatment

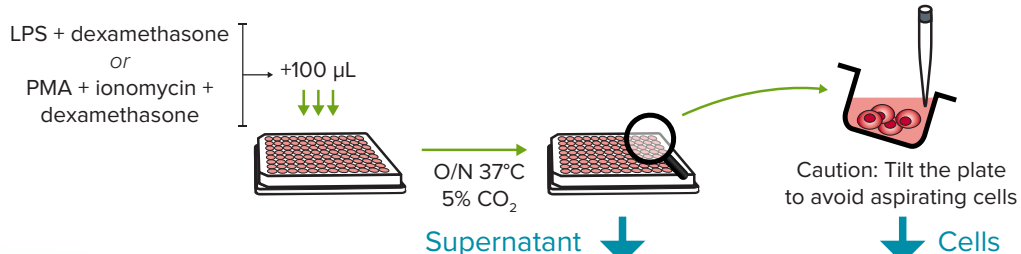


3 HTRF cytokine assays

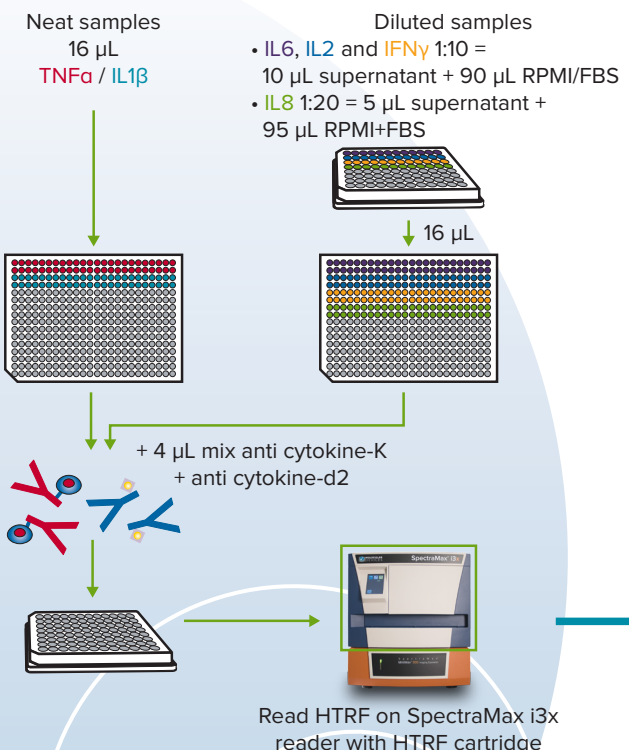

4 EarlyTox assay

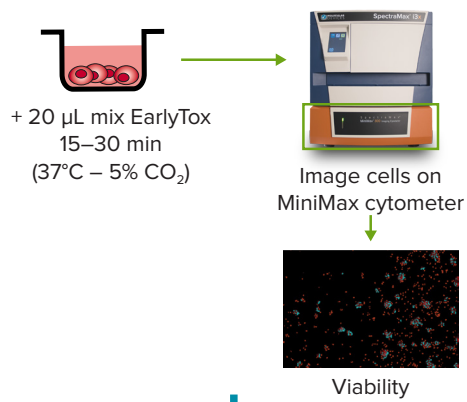

5 Normalization



The normalized concentration of cytokines is expressed in pg/mL per living cell.

For more information on the SpectraMax i3x reader with MiniMax cytometer, please visit moleculardevices.com/i3x

www.moleculardevices.com | 800.635.5577

©2018 Molecular Devices, LLC The trademarks used herein are the property of Molecular Devices, LLC or their respective owners. Specifications subject to change without notice. Patents: www.moleculardevices.com/productpatents FOR RESEARCH USE ONLY. NOT FOR USE IN DIAGNOSTIC PROCEDURES. 1/18 Printed in USA

